



KONICA MINOLTA

MEDICAL DUPLICATING FILM

SR Dup_{PLUS}

D · U · P · L · I · C · A · T · I · N · G




The essentials of imaging

MEDICAL DUPLICATING FILM SR Dup_{PLUS}

For 1:1 Reproduction of Medical X-ray Radiographs.

Characteristic curves

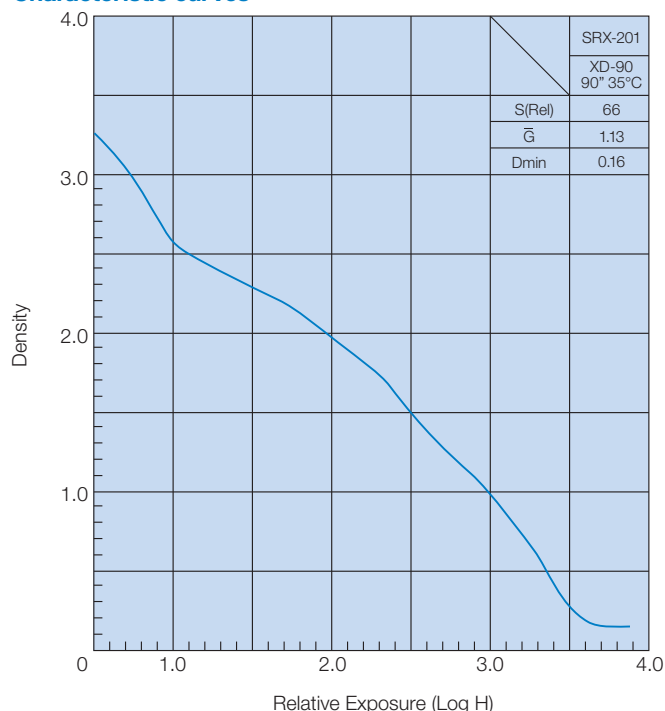

This graph shows typical response to SR Dup PLUS FILM exposed under ultraviolet light sources.

MEDICAL DUPLICATING FILM SR Dup PLUS is specifically designed to produce uniform linearity in image reproduction. In fact, copies are so authentic it may be difficult to tell the original from the reproduction. SR Dup PLUS FILM features a non-glare matte finish on both sides.

Specially Designed and Compatible for use with Ultraviolet Light

SR Dup PLUS film features high low density contrast. It also features a high density contrast level of 1.0 and a minimum density of 0.16. It provides excellent reproduction quality over a wide range of film density. SR Dup PLUS produces a maximum density of 3.0. These specifications make this an ideal medium for faithful reproduction of both conventional x-ray photographs and clinical images from MRI, CT and other sources.

Handling

Like all radiographic films, SR Dup PLUS FILM should be handled with care to avoid artifacts.

Safelight Recommendations

SR Dup PLUS film can be used with conventional safelight filters. Light source should not exceed a single 15 watt bulb at a distance of at least 4 feet (1.2m).

*Recommended: Sylvania 350 Black Light-F15T8/350 BL Model.

*Specifications are subject to change without notice.

Konica Minolta medical film is manufactured with a quality management system that has been certified to be in compliance with the ISO 9001:2000 and ISO 13485:2003 quality management standards, as well as with the medical device directive (MDD) 93/42/EEC.



KONICA MINOLTA

KONICA MINOLTA MEDICAL IMAGING USA, INC.

411 NEWARK POMPTON TURNPIKE, WAYNE, NJ, 07470, USA

Tel: (973) 633-1500 Fax: (973) 633-0562, medical.konicaminolta.us

Distributed by: