




KONICA MINOLTA

Traceability System for TV-, CRT- and Display-Color Analyzer

January, 2004

Konica Minolta Photo Imaging Europe GmbH
Instrument Systems Division

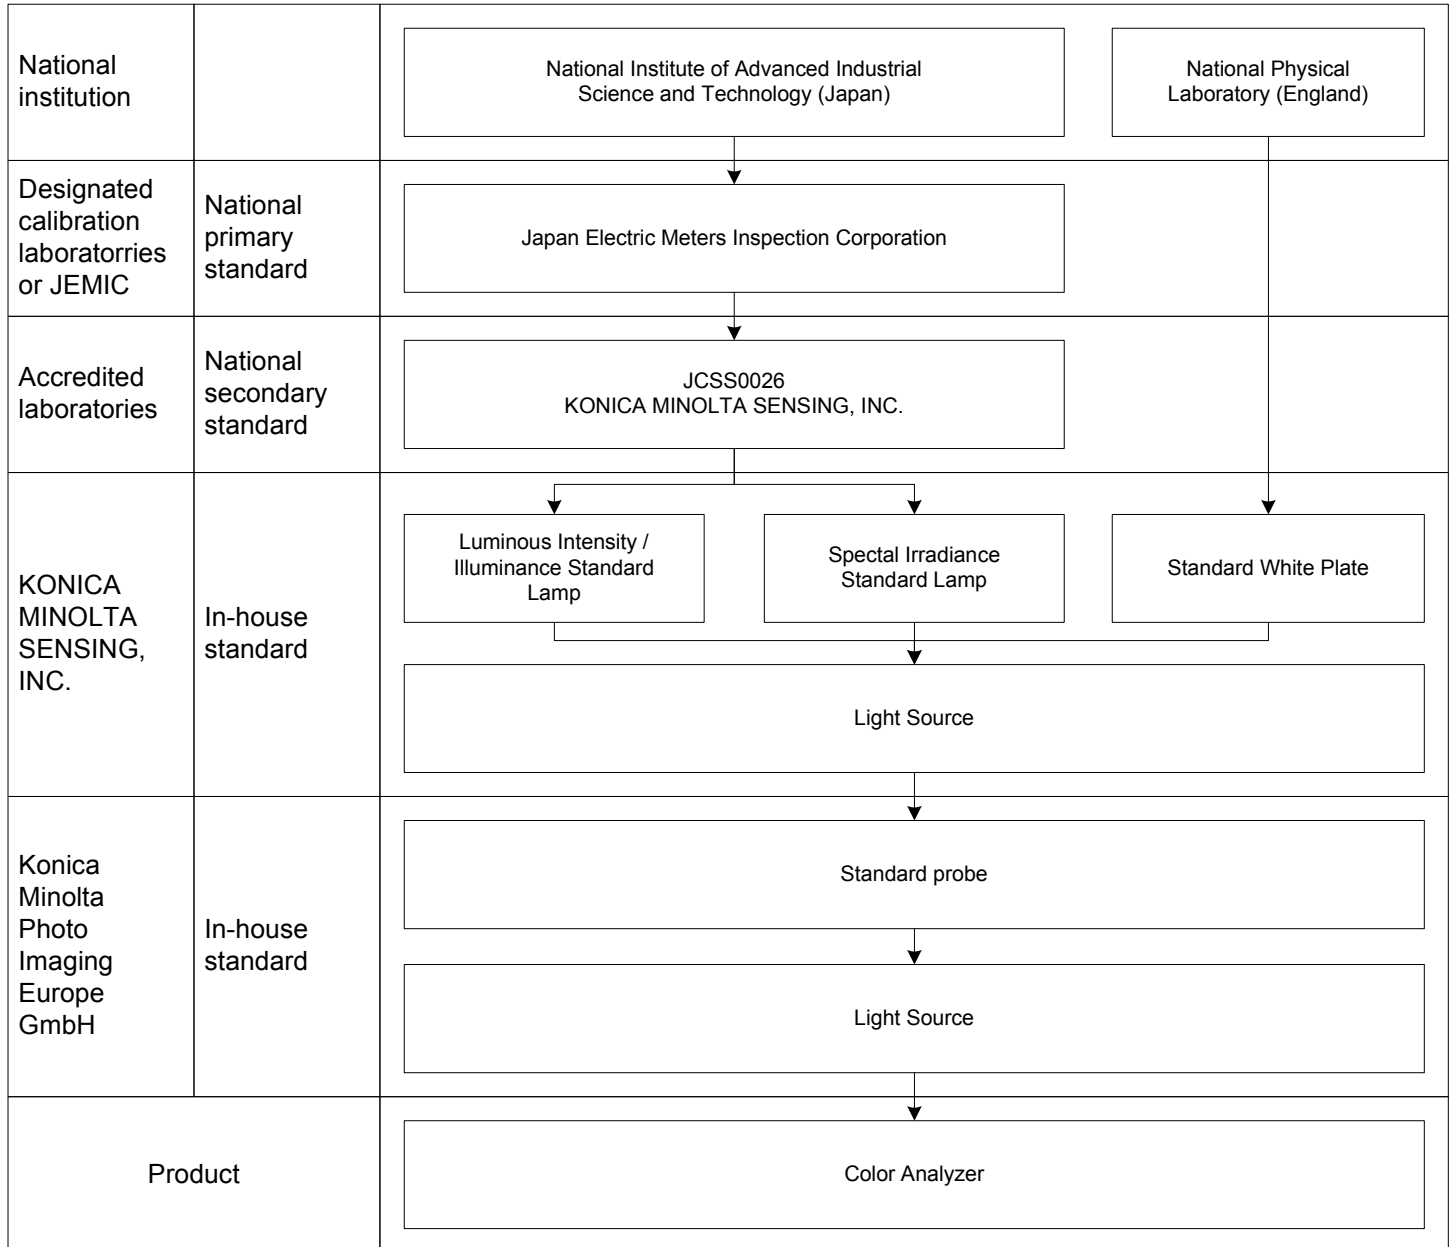

Interval between calibration:

Luminous Intensity / Illuminance Standard Lamp: 1 year or 10 hours of accumulated use

Spectral Irradiance Standard Lamp: 1 year or 10 hours of accumulated use

Standard White Plate: 5 years

Light Source: Each time the product is calibrated

Standard probe : 1 year

JCSS0026: Japan Calibration Service System, the calibration laboratory accreditation system in Japan.

The organization number for KONICA MINOLTA SENSING, INC. is 0026